Multiple Run Fitter

Goal: Adjust model parameters to fit data from multiple experiments.

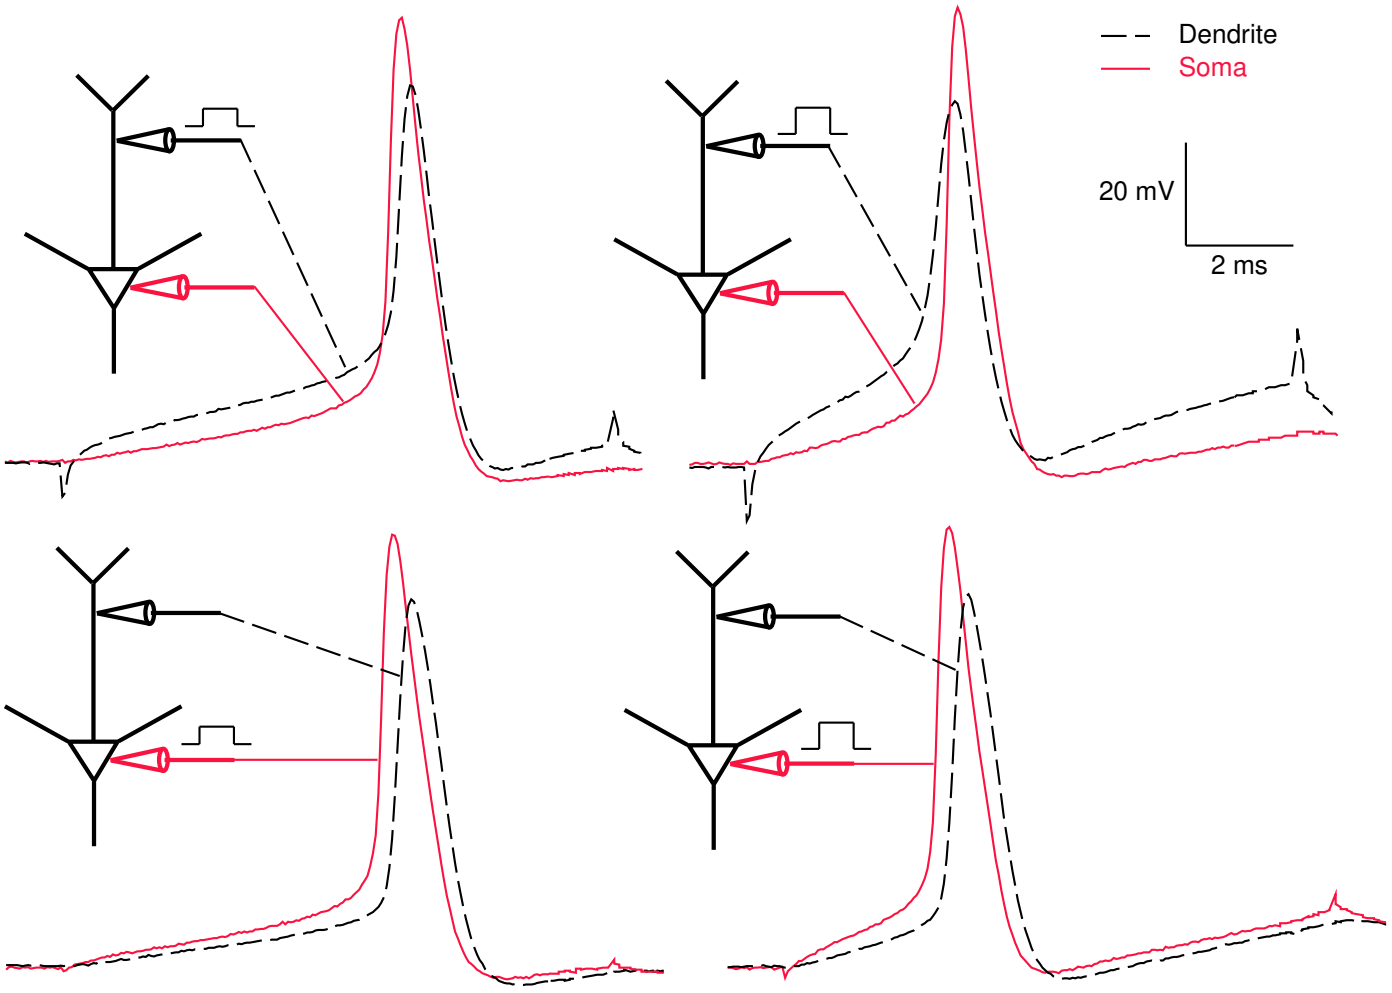

See: Shen et. al. (1999), J. Neurophysiol. 82:3006
Computational analysis of action potential initiation in mitral cell soma and dendrites based on dual patch recordings.